



## Inline Air Walker

Single Patient Use Only

Rx Only



### IMPORTANT INFORMATION

Please read all instructions before use. Correct application is essential to proper functioning of product.

### INDICATIONS


Grade 2 and 3 ankle sprains; stable fractures of tibia, fibula, talus and tarsus; post operative immobilization (soft tissue reconstructions and open reduction internal fixation); metatarsal fractures

### PRECAUTIONS


- This product is to be fitted initially by a physician (or properly licensed practitioner) who is familiar with the purpose for which they are responsible. The physician or practitioner is responsible for providing use instructions and precautions to other healthcare practitioners, care providers involved in the patients' care and the patient.
- Consult your physician (or properly licensed practitioner) immediately if you experience sensation changes, unusual reactions, swelling or prolonged pain while using this product.
- Follow the instructions of your physician (or properly licensed practitioner) for length and duration of use.

### INSTRUCTIONS FOR USE

1. Remove inner liner/wrap from walker. Position foot and lower leg into the liner.



2. Wrap snugly around limb. Fasten with "hook" fasteners to the outside of liner. Insert foot and lower leg into walker.
3. Carefully center the uprights (side panels) over the ankle to ensure a comfortable fit and proper support. Remove covers from uprights and secure liner.
4. Remove inflator bulb from front pocket on liner. Inflate air bladder per physician's order by inserting clear end of inflation/deflation bulb into air valve and squeezing.
5. Once desired compression is achieved, fasten walker using hook and loop leg straps. Begin fastening at the bottom and work your way up the leg.
6. Check for adequate circulation. Readjust straps and air amount as

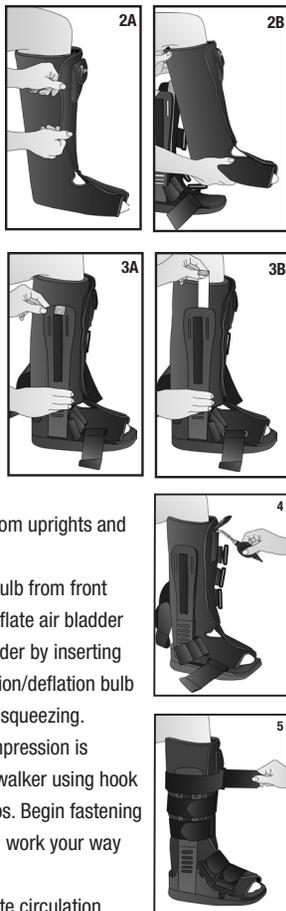

## Inline Air Walker

Single Patient Use Only

Rx Only



### IMPORTANT INFORMATION

Please read all instructions before use. Correct application is essential to proper functioning of product.

### INDICATIONS


Grade 2 and 3 ankle sprains; stable fractures of tibia, fibula, talus and tarsus; post operative immobilization (soft tissue reconstructions and open reduction internal fixation); metatarsal fractures

### PRECAUTIONS


- This product is to be fitted initially by a physician (or properly licensed practitioner) who is familiar with the purpose for which they are responsible. The physician or practitioner is responsible for providing use instructions and precautions to other healthcare practitioners, care providers involved in the patients' care and the patient.
- Consult your physician (or properly licensed practitioner) immediately if you experience sensation changes, unusual reactions, swelling or prolonged pain while using this product.
- Follow the instructions of your physician (or properly licensed practitioner) for length and duration of use.

### INSTRUCTIONS FOR USE

1. Remove inner liner/wrap from walker. Position foot and lower leg into the liner.



2. Wrap snugly around limb. Fasten with "hook" fasteners to the outside of liner. Insert foot and lower leg into walker.
3. Carefully center the uprights (side panels) over the ankle to ensure a comfortable fit and proper support. Remove covers from uprights and secure liner.
4. Remove inflator bulb from front pocket on liner. Inflate air bladder per physician's order by inserting clear end of inflation/deflation bulb into air valve and squeezing.
5. Once desired compression is achieved, fasten walker using hook and loop leg straps. Begin fastening at the bottom and work your way up the leg.
6. Check for adequate circulation. Readjust straps and air amount as

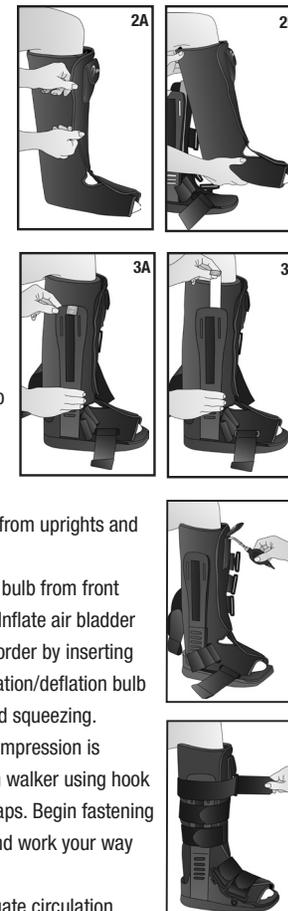

DeRoyal®

needed for a secure and comfortable fit. **NOTE:** To deflate air bladder, insert black end of inflation/deflation bulb into air valve and squeeze bulb to deflate bladder.



DeRoyal®

**Manufactured by DeRoyal**  
200 DeBusk Lane  
Powell, TN 37849 U.S.A.  
888.938.7828  
865.938.7828

Part#0-InlineWalkerInsert  
©2007 DeRoyal. All Rights Reserved.  
Revised 1/07

**WASHING INSTRUCTIONS**

Liner should be hand washed using cold water and mild detergent. Air dry.

**MediRoyal Nordic AB**

Staffans väg 6 B, S-192 07 Sollentuna SWEDEN

+46 8 506 766 00

[www.mediroyal.se](http://www.mediroyal.se)

DeRoyal®

needed for a secure and comfortable fit. **NOTE:** To deflate air bladder, insert black end of inflation/deflation bulb into air valve and squeeze bulb to deflate bladder.



DeRoyal®

**Manufactured by DeRoyal**  
200 DeBusk Lane  
Powell, TN 37849 U.S.A.  
888.938.7828  
865.938.7828

Part#0-InlineWalkerInsert  
©2007 DeRoyal. All Rights Reserved.  
Revised 1/07

**WASHING INSTRUCTIONS**

Liner should be hand washed using cold water and mild detergent. Air dry.

**MediRoyal Nordic AB**

Staffans väg 6 B, S-192 07 Sollentuna SWEDEN

+46 8 506 766 00

[www.mediroyal.se](http://www.mediroyal.se)